



RCaMP2 configuration filter set

Application Note

© 2021 DORIC LENSES INC



357 rue Franquet - Quebec, (Quebec)

G1P 4N7, Canada

Phone: 1-418-877-5600 - Fax: 1-418-877-1008



www.doriclenses.com

basic fluorescence microscope: Filter set for RCaMP2 excitation

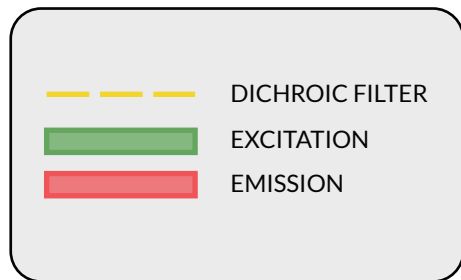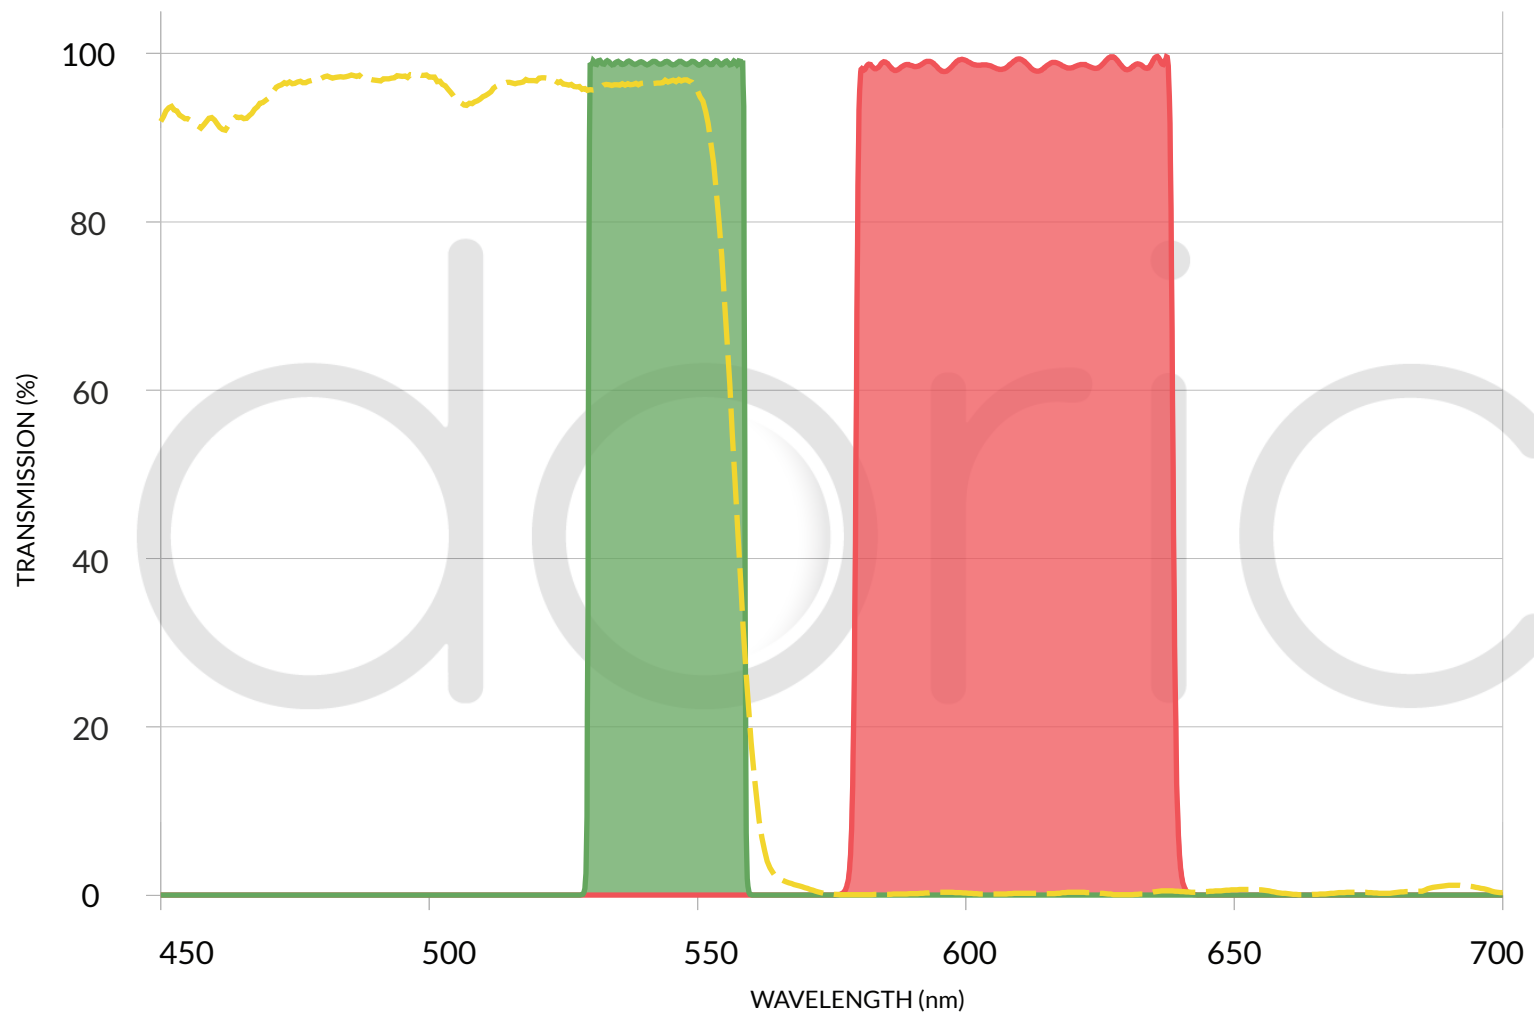

doric

BASIC MICROSCOPE FILTER SET DIAGRAM

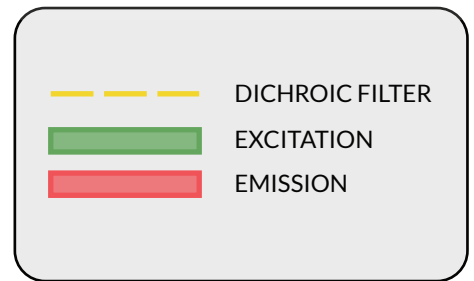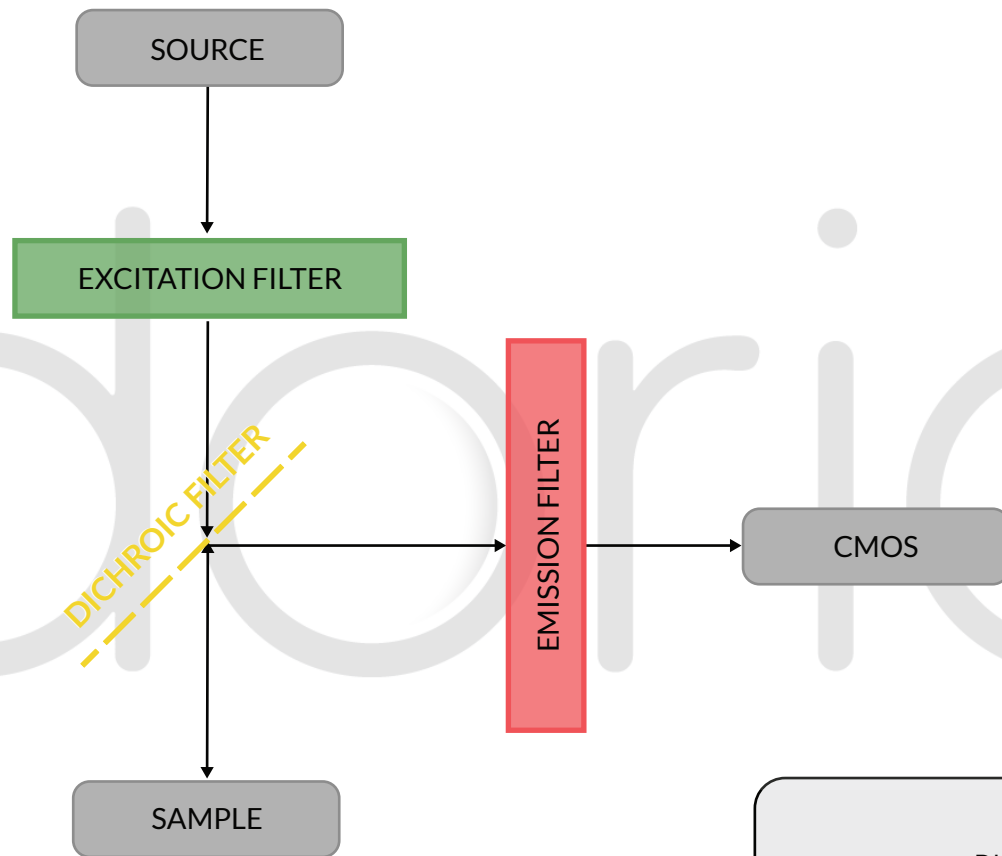

doric